

## TECHNICAL BULLETIN

---


At times there is high pressure inside the elastomeric bladder that creates resistance when filling the pump. However, with enough force applied, the pressure will be overcome and the pump can continue to be filled. Please note that asymmetrical filling of the pump may also cause resistance during filling once one side has completely filled and the other begins to expand. Asymmetrical filling, however, does not affect the functionality of the device.

The following steps should be followed when using a syringe in order to correctly fill an elastomeric pump manufactured by Halyard Health.

1. Remove the cap from the fill port and retain for later use.
2. The elastomeric pump should be filled with a 60cc syringe or similar device.
3. Remove all air from the filling device and attach it securely to the pump fill port.
4. After attaching syringe to the fill port, invert pump as shown below. Firmly grasp the syringe with both hands and push down on the plunger continuously until the volume is dispensed. Resistance may be felt. Repeat as necessary in order to fill the pump completely.

**Do not push down on the pump while filling as the syringe tip may break.**

5. Remove filling device from the fill port and securely replace the fill port cap.

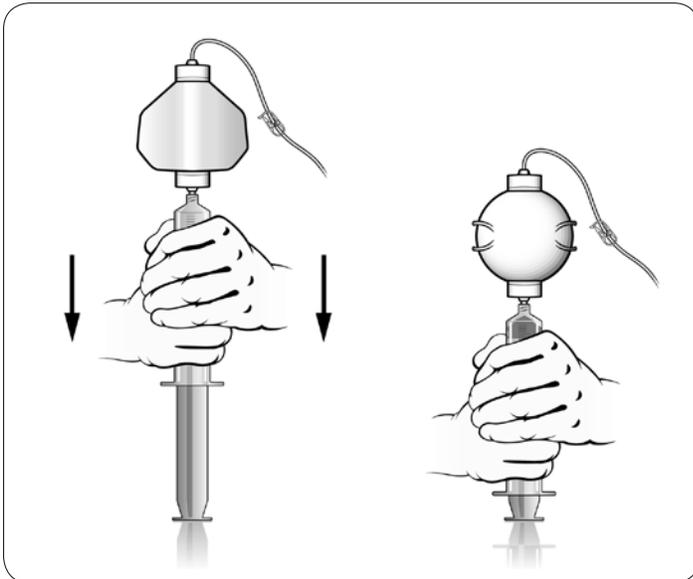

---

There are inherent risks in all medical devices. Please refer to the product labeling for **Indications, Cautions, Warnings and Contraindications**. Failure to follow the product labeling could directly impact patient safety. Physician is responsible for prescribing and administering medications per instructions provided by the drug manufacturer. Refer to [www.halyardhealth.com](http://www.halyardhealth.com) for additional product safety **Technical Bulletins**.

Please contact the Clinical Services Department at **800-444-2728** or **949-923-2400**  
if you have any questions regarding this information.

---